

# High Precision Calibration Source for Voltage, Current and Thermocouple DIGISTANT®

Type 4462

Code: 4462 E  
 Manufacturer: burster  
 Delivery: upon request  
 Warranty: 12 months  
 Issue: 1.3.2000



- High precision current and voltage source  $\pm 52$  mA,  $\pm 30$  V
- Precision simulation for all conventional thermocouple types (optional)
- Basic accuracy 0.005 % of reading
- RS232- and optional IEEE488 interface

## Application

The precision calibration unit combines high accuracy, low drift, low noise and superior long-term stability with multiple functionality and simple operation.

Ramps,  $\Delta+$ / $\Delta-$ , and multiple setpoint storage make the operation of the device easier for the user.

For that reason the application possibilities are many:

- Testing current and voltage meters
- Precise testing of thermocouple temperature measuring instruments
- Calibration of controllers, sensors, detection devices and other devices used in process control
- Open-loop process control with the aid of integrated ramp functions.

The DIGISTANT® type 4462 can be used both as a stand-alone table-top device, as well as in automatic, computer-assisted manufacturing and testing systems.

## Description

It is possible to set currents of  $\pm 200$  nA ...  $\pm 52$  mA, voltages of  $\pm 1$   $\mu$ V ...  $\pm 30$  V and, optionally, temperature setpoint values of 14 thermocouple types.

The output value is fed back via the sensor line to eliminate voltage drops across the measuring leads.


The device has an adjustable current/voltage limitation. An external voltage divider of 1 up to 1:1000 can be considered internally.

With the thermovoltage sourcing option you can enter °C, °F and K, the temperature scales ITS 90 or IPTS 68 and the comparison point mode constant/external. Furthermore, when sourcing thermocouples a calibrated external comparison point can be used, whereby the data for calibration in the device can be taken into consideration.

Indication of the source value is carried out in large 12 mm figures on an illuminated graphics-LCD.

The device can be operated both via the keyboard as well as the interface.

**Source main menu**

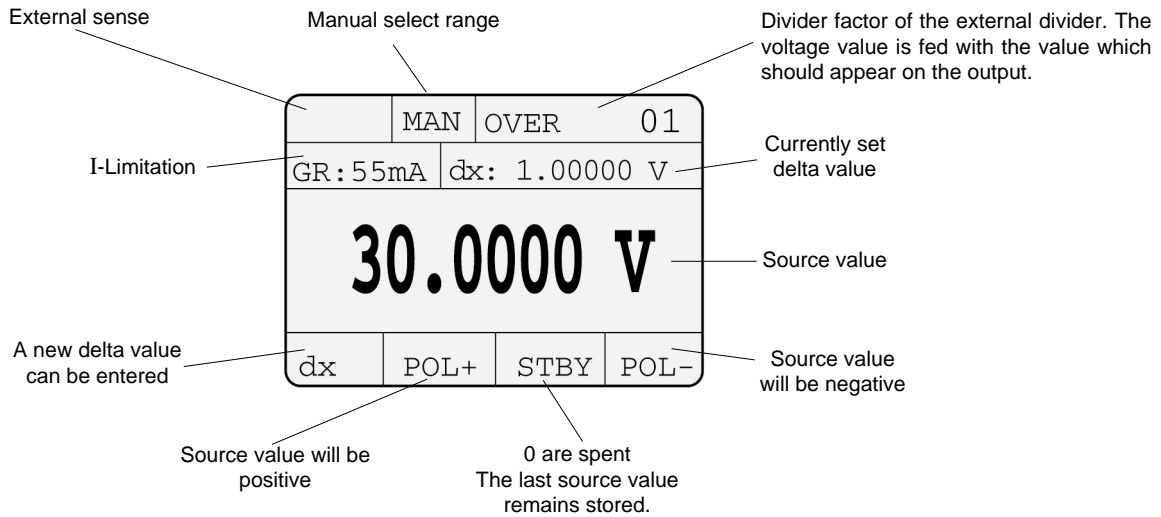

**Operation Examples**

**Ramp 1 Configuration menu**

<b>SEQUENZ: TRIANGEL</b>			
REPETITIONS: 17			
START-VAL.: 0.0mV			
END-VAL.: 250.0mV			
DELTA-VAL.: 25.0mV			
DELTA-TIME. hh:mm:ss.s			
			RETU

**Ramp Function:**

- Ramp 1 with constant delta values and delta time
- Ramp 2 with variable delta values and interval time.

The ramp function allows single or repeated outputs in sawtooth or triangular form. The number of steps can set from 0 to 99 (0 is continuous). The START, END and DELTA values can be entered in  $\mu$ V, mV, V, mA and temperature values. DELTA time is displayed as shown in the menu.

**Current/Voltage limit setting**

LIMITATION			
<b>U-LIMIT: 20V</b>			
I-LIMIT: 10mA			
1 V >----< 32V			
		HOME	RETU

**Current/Voltage Limit:**

If a voltage or temperature value is given, the current limit is automatically active. At the current source the voltage limit is active. The U-limit ranges from 1V to 32V and the I-limit ranges from 1 mA to 55 mA.

**TC/Temperature menu**

<b>TC-TYPE: K IPTS68</b>			
RJ-TYPE: EXTERN			
RJ-TEMP: 300.00K			
TEMP.DIMENSION: K			
SKALE: IPTS68			
		HOME	RETU

**Pt 100 Scale  
(Measurement with external RJ)**

<b>A = 0.0039083</b>			
Ro = 100			
B = -5.775E-07			
C = -4.183E-12			
DIN EN: 0.0039083			
0.003 < -- > 0.006			
Exp	EN	HOME	RETU

Optionally the thermocouples types R, S, B, J, T, E, K, U, L, N, M, C, D and G2 can be simulated. For the "manual" reference junction at 0 °C the accuracy depends on the thermocouple type starting at 0.1K. The connection ensues "manually" directly at the standard terminals and "externally" via an external, attachable reference junction type 4485-V001, at which the temperature is detected with a Pt 100 sensor (see application).

**Technical Data**

**Voltage Source**

Range ±	Resolution	Error limits at 23°C ± of reading	TC with resp. to 23 °C
30 V	0.1 mV	0.003% (to ± 4.5 V) +200 μV (>± 4.5 V) +1.1mV	8ppm/K +10μV/K
3 V	10 μV	0.003% (to ± 450 mV) +20 μV (>± 450 mV) +110 μV	8ppm/K +1μV/K
300mV	1 μV	0.003% (to ± 45 mV) +3 μV (>±45 mV) +11 μV	8ppm/K +0,35μV/K

Output current: max. 52 mA at 30 V

**Current source**

Range ±	Resolution	Error limits at 23°C ± of reading	TC with resp. to 23 °C
52 mA	200 nA	0.007% (to ± 7.5 mA) +0.6 μA (>± 7.5 mA) +3 μA	10ppm/K+10nA/K

Burden voltage: max. 30 V at 52 mA

Confidence coefficient for the specified errors: 95% (K=2).

**Option: Thermocouple simulation**

Type	Range	Error (K)
R	+ 250 ... 1768 °C	0.4 (+ 250 ... 1768 °C)
S	+ 350 ... 11768 °C	0.4 (+ 350 ... 1768 °C)
B	+ 800 ... 1820 °C	0.5 (+ 800 ... 1820 °C)
J	- 210 ... 900 °C	0.2 (- 210 ... 900 °C)
T	- 170 ... 400 °C	0.2 (-170 ... 400 °C)
E	- 220 ... 1000 °C	0.2 (- 220 ... 1000 °C)
K	- 50 ... + 800 °C	0.1 (- 50 ... 800 °C)
U	- 100 ... + 600 °C	0.3 (- 100 ... 600 °C)
L	- 100 ... + 750 °C	0.2 (- 100 ... 750 °C)
N	- 120 ... 1200 °C	0.2 (- 120 ... 1200 °C)
M	- 50 ... + 900 °C	0.1 (- 50 ... 900 °C)
C	100 ... + 900 °C	0.2 (+ 100 ... 900 °C)
D	+ 300 ... 1100 °C	0.2 ( 300 ... 1100 °C)
G2	+ 300 ... 2100 °C	0.3 ( 300 ... 2100 °C)

The errors are defined at "manual" reference junction 0 °C. The connection performed "manually" direct at the standard sockets: The external reference junction type 4485-V001 may be stick up, the temperature is measured with a Pt 100 sensor (see application No.1).  
If you enter the probe calibration data (NAMAS, DKD and others) the accuracy of the temperature measurement is better than ≤ 0.1 K (Operating temperature 15 ... 35 °C).

**Option: Temperature measurement with Pt 100 (without sensor)**

Range	Resolution	Current (mA)	TC with resp.
- 200 ... 850 °C	0.01 K	approx. 0.6	0.00006* T+0.045 K

T = temperature in °C

Internal resistance: Voltage source < 10 mΩ  
Current source > 500 MΩ

Long-term stability: U-Drift < 20 ppm / year + 2 μV / year (300 mV)  
U-Drift < 20 ppm / year + 6 μV / year (3 V)  
U-Drift < 20 ppm / year + 10 μV / year (30 V)  
I-Drift < 70 ppm / year + 0,5 μA / year

Warm-up time: 30 minutes, until specified error limit  
External divider: 1 to 1010  
Current limitation: for U up to 30 V 1 mA ... 50 mA  
Voltage limitation: for I up to 50 mA 1 V ... 30 V  
Display: Graphics LCD display, with LED illumination


Visual field: 56,3 mm x 38 mm, resolution 128 x 64 dots  
Sockets: + output, - output, + sensor, - sensor, gold-plated 4 mm-terminals and a 6-pin LEMO socket 1B for the optional Pt 100 connection  
Device construction: Metal housing in protection class I in accordance with DIN EN 61010 part 1  
Power supply: 230 V ± 10 %, 45 Hz ... 65 Hz, can be changed on device to 115 V  
Power requirement: approx. 30 VA  
Dimensions: (L x W x H) 237 x 285 x 151 [mm] (with handles W = 325 mm)  
Weight: approx. 6 kg

**Outputs and Terminals on the Rear Side**

Standard RS232C interface: 9-pin subminiature D-socket  
Baud rate 300 - 38 400  
Protocol ANSI X 3.28 1976  
Subcategory 2.1, A3  
Optional IEEE488 interface: 24-pin, open collector outputs (E1) SH1, AH1, T6, TE0, L4, LE0, SR1, RL1, PP0, DC1, DT1, C0  
Instruction language: SCPI, Version 1997.0

**Order Information**

**DIGISTANT®**



Standard with RS232

Additional with IEEE488

Option thermocouple simulation  
RJ-Temp. recording (temperature measurement with Pt 100)  
Subsequent mounting possible

**Accessories**

- 4 measuring leads with low thermal voltage Cu/Te safety connectors, length 1 m **type 6706-K001**
- RS232 data cable** for PC connection **type 9900-K333**
- Assembly set for 19" rack mounting** **type 2329-Z004**
- External reference junction for DIGISTANT® type 4462** **type 4485-V001**

**Calibration Certificates for Type 4462**

**DKD Calibration (Basic system)**  
Each range (voltage, current) is calibrated at ± 12,5%, 25%, 50% and 90% of full scale. **Order code 44DKD-V100**


**DKD Calibration (Extended system)**  
Each range (voltage, current) is calibrated at ± 12,5%, 25%, 50% and 90% of full scale.  
With 2 points for 10 thermocouples, temperature of the reference junction 0 °C. **Order code 44DKD-V110**

**Calibration Certificates for type 4485-V001 DKD Calibration**  
for the external reference junction at 3 points (0 °C, + 23 °C and + 40 °C) **Order code 44DKD-4485**


## Application Examples

### 1. Calibration of a PC card with a thermocouple measurement input

Instead of the thermocouple the calibration source DIGISTANT® type 4462 is connected. Using an external DKD-calibrated reference junction the PC card is retraceably calibrated with the optimum accuracy. Up to 14 thermocouples can be selected.

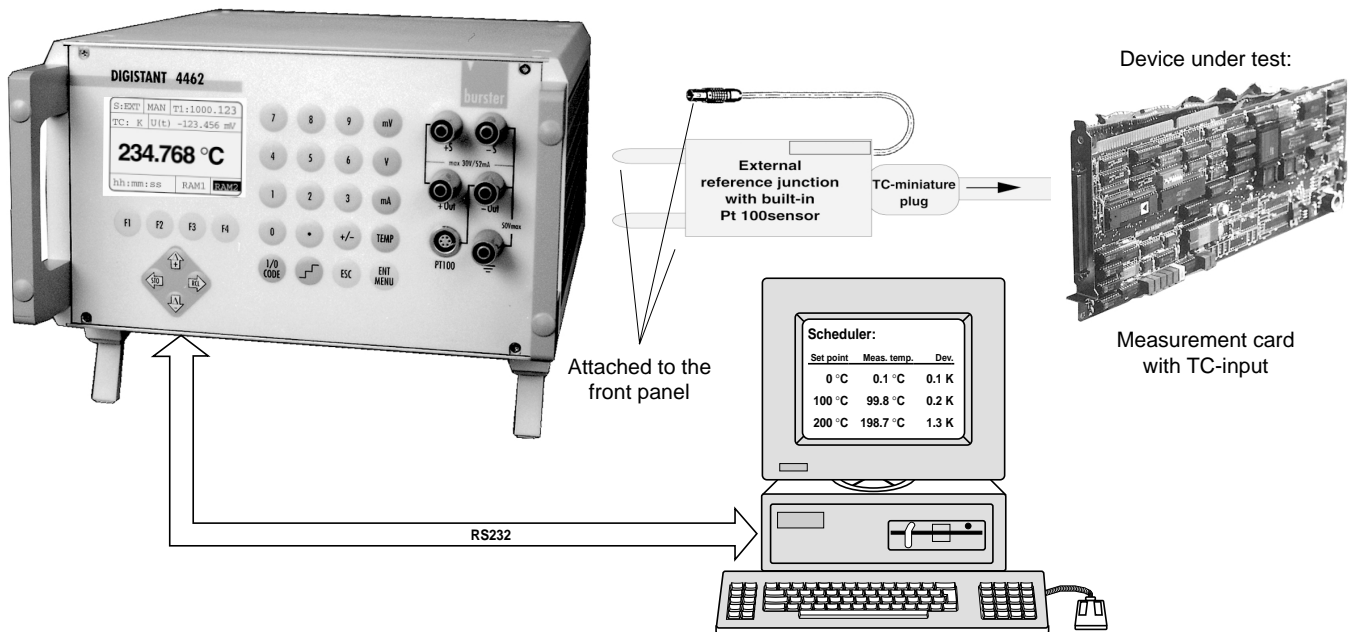


### 2. Calibration of measuring system in the medicine engineering

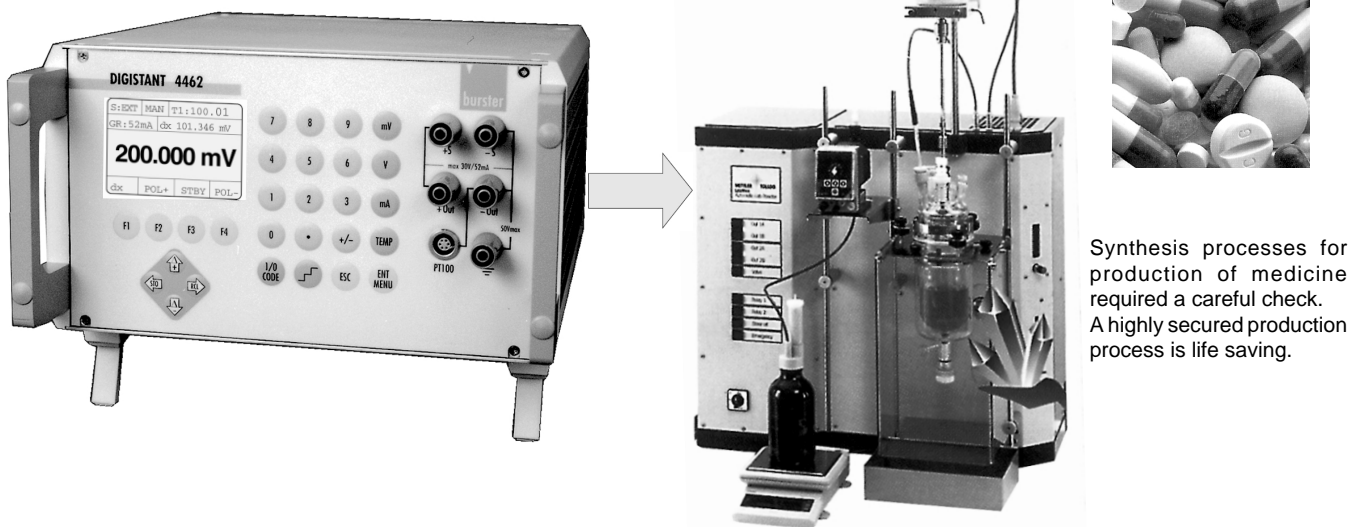

### 3. Calibration of a recorder

In the sweep function you set different current and voltage values with individual steps. The output happens once or repetitioned in triangular or sawtooth wave.

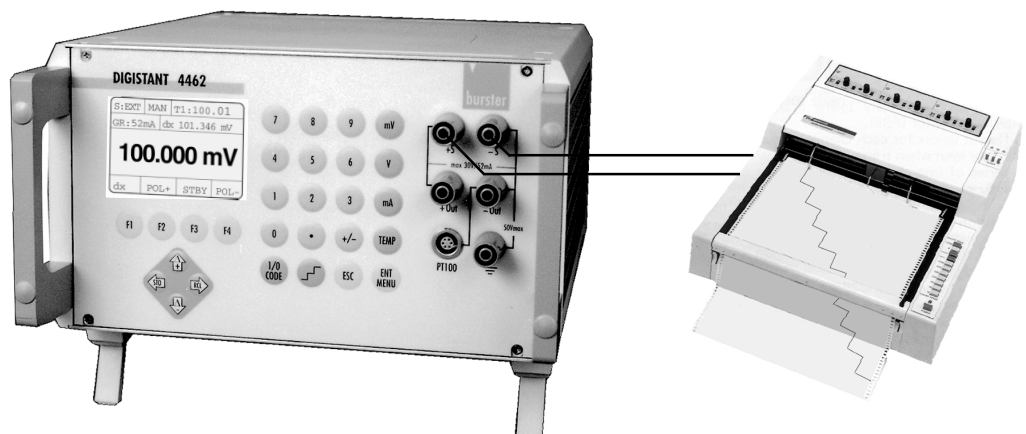

Technical alterations reserved